

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

APR 05 2010

Supervisor/Operator Performing the Verification Procedure:

DataMaster cdm S/N 130183

A

Name Hutt, William T

ID# 3359

Date 2/28/10

Agency HOMER POLICE DEPT / JAIL

Phone # 235-3150

Instrument Location 4060 HEATH ST. HOMER AK 99603

B

Alco S/N A090740

Target Value .084

High Pressure 100 PSI

Alco Test Value Average .081
1st Alco

.080
2nd Alco

Signature

William T. Hutt

(OVER)

BMB
4/8/10

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
Nita J. Bolz

Scientific Director

State Breath Alcohol Program



Subscribed and sworn before me this 15th day of April, 2010.

(Notary Seal Stamp)

Carolyn M. Noland
Carolyn M. Noland

Notary Public, State of Alaska

Commission Expires with Office

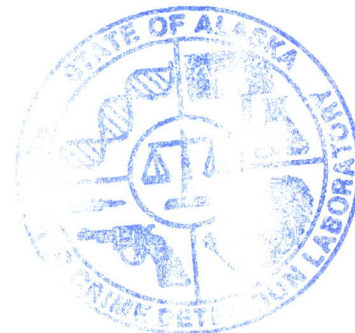

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130183

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130183 ✓

FEBRUARY 28, 2010 ✓

OPERATOR'S NAME:
HUTT, WILLIAM T
OPERATOR'S NUMBER: 3359
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
ETOH

O.L. #: 01234567
DEPT/AGENCY: HOMI
CASE/REPORT: 10-0000
TEST TYPE: U
ALCO TARGET VALUE: 0.004 ✓
ALCO S/N: 0090740 ✓

— BREATH ANALYSIS —

.004 ADJUSTED FOR 28.89 in ✓
ALCO TARGET .001 20:31
BLANK TEST .000 20:32
INTERNAL STANDARD VERIFIED 20:32
ALCO TV 28.89 in .001 20:33
BLANK TEST .000 20:33
SUBJECT SAMPLE .000 20:34
BLANK TEST .000 20:35
ALCO TV 28.89 in .000 20:36
BLANK TEST .000 20:37

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130183 ✓

FEBRUARY 28, 2010
TIME 20:27

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 28.89 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ ¡ ¢